

SERIES 5 EURO-STYLE DELIVERY SYSTEM ON A DCI EDGE SERIES 5 CHAIR

Installation Instructions

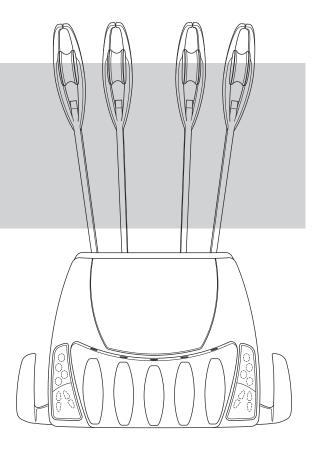

SERIES 5 EURO-STYLE DELIVERY SYSTEM Installation Instructions

OVERVIEW

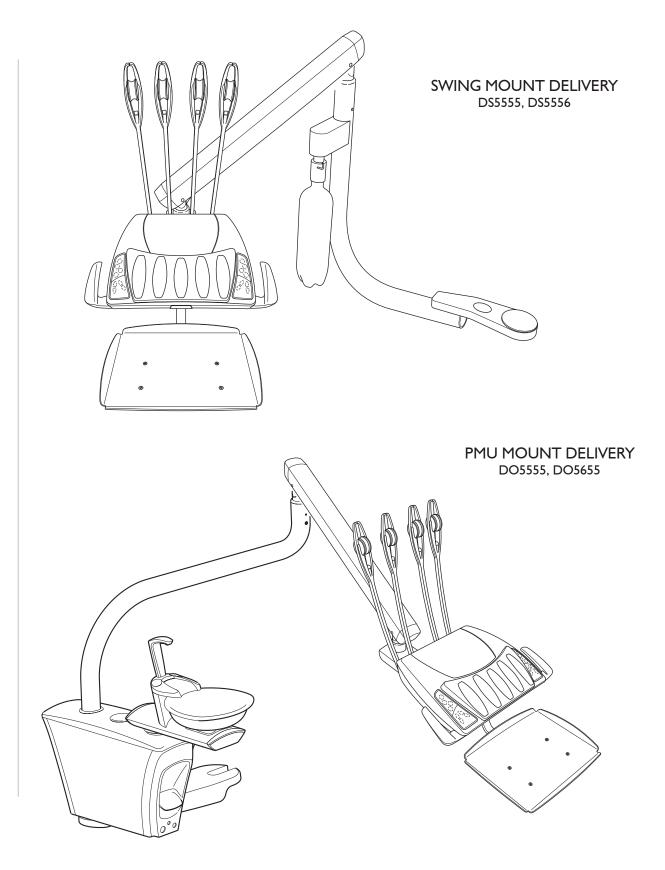

2 DCI Edge

INTRODUCTION

BEFORE YOU BEGIN

Study the unit overview in this booklet and layout dimensions from the owner's manual. Make sure the planned location will have the necessary space available for installation, including room for travel of the chair's base and backrest.

Open all containers and review the contents. It may be helpful to locate all kits containing accessories. (Smaller parts are often packaged together to avoid being lost.)

Locate all documentation supplied with the package. Manuals and installation sheets may be found in one or more boxes accompanying their respective components. Set aside the owner's manual for the end user to review.

If a complete ensemble is to be installed, set up the chair first. Refer to the installation manual supplied with the chair for instructions.

In all configurations, the unit pole, unit flex arm, and unit control head come shipped as a complete assembly. In some of the following illustrations, only the unit pole may be shown for clarity.

TABLE OF CONTENTS

Overview	2
----------	---

- Introduction 3
- PMU Mount Installation 4
- Swing Mount Installation 9
- Managing the Umbilical 13
 - Junction Box Layout 14
 - Make Connections 15 and Adjustments

SYMBOLS USED IN THIS MANUAL

The following symbols may be used throughout this product manual:



WARNING: Failure to carefully follow the described procedure may result in damage to the equipment or the operator.



CAUTION: Failure to carefully follow the described procedure may result in damage to the equipment.



NOTE: Take note of additional important information. Not a warning or caution.



ELECTRICAL HAZARD: Risk of electrical shock present. Ensure that power is disconnected before attempting procedure.


REGULATORY INFORMATION

Regulatory information is delivered with DCI Edge dental equipment as mandated by agency requirements and can be found in the accompanying Instructions for Use for this device.

PMU MOUNT UNIT INSTALLATION

TOOLS NEEDED FOR INSTALLATION

Socket wrench Socket wrench extension (3") 9/16" and 3/4" Sockets Magnetic Level Allen wrench set Utility knife

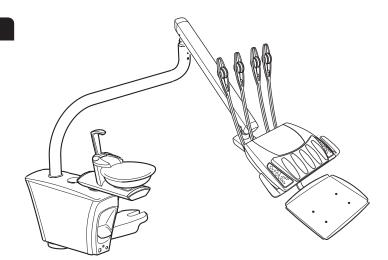

INCLUDED HARDWARE

4 Hex bolts 3/8"-16 x 1 1/4"


4 Lock washers 3/8"

PREPARATION

Ensure that the dental chair has been completely set up and in its final location.

2 Remove the shipping bolt from the chair.

Install the power switch cover.

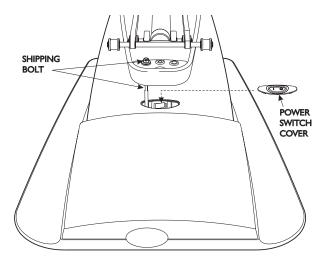


3

PMU MOUNT UNIT INSTALLATION

MOUNTING TO THE CHAIR

Assemble the hanging bolt and washer to the underside of the seat casting, ensuring that at least 1/2" of the screw thread is exposed.

2 Slide the PMU Mount Casting and Post Assembly on the hanging bolt and position it so that it is perpendicular to the seat casting.

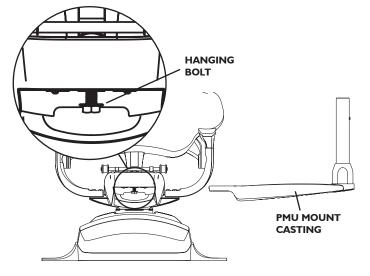



WARNING: To prevent injury, have an assistant support the weight of the unit and mount casting during installation.

Align the holes on the PMU Mount Casting to the 4 holes of the Seat Casting. Assemble the 4 3/8" hex bolts from above, by dropping them through the four holes in the seat casting as shown and turn them in part way by hand.


Tighten using a 9/16" socket wrench with a socket extension.

5 Measure the level of the assembly by attaching a magnetic level to the front of the post and then at the side of the post.

6 Adjust the level by loosening the 4 3/8" hex bolts by at least 2 full turns and then tightening the 3 set screws circled in the illustration (right) as needed. Retighten the 4 hex bolts and recheck the level.

7 Complete the process by tightening the bottom Hanging Bolt with a 3/4" socket and wrench to secure the leveling.


WARNING: Before using of the equipment, ensure that the assembly is level and all mounting bolts are securely fastened.

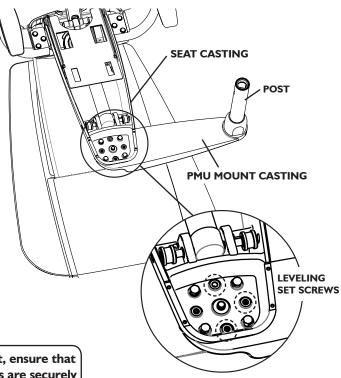

PMU MOUNT UNIT INSTALLATION

ATTACHING THE PMU


Assemble the PMU box onto the post by aligning the post with the large socket in the internal PMU casting as shown (below) and dropping the casting down over the post until it is seated securely. Rotate the PMU to be parallel to the chair until you feel it lock into position as a pin on the post engages in a slot in the casting.

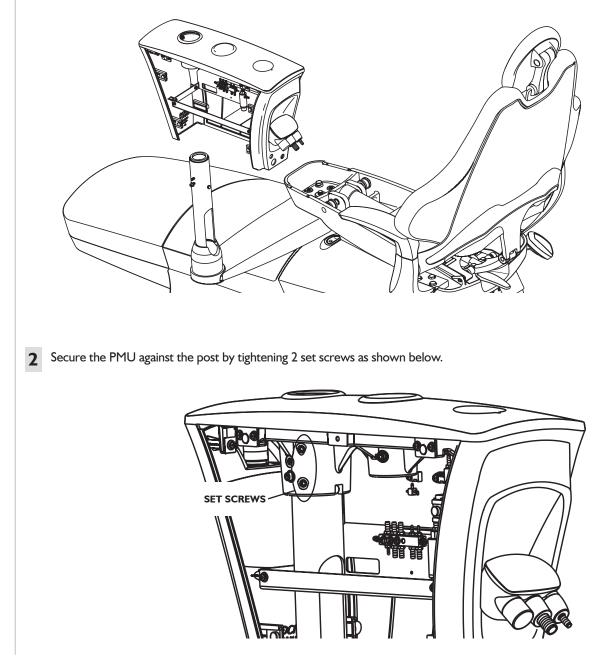

S-POLE


PMU MOUNT UNIT INSTALLATION

ATTACH THE S-POLE

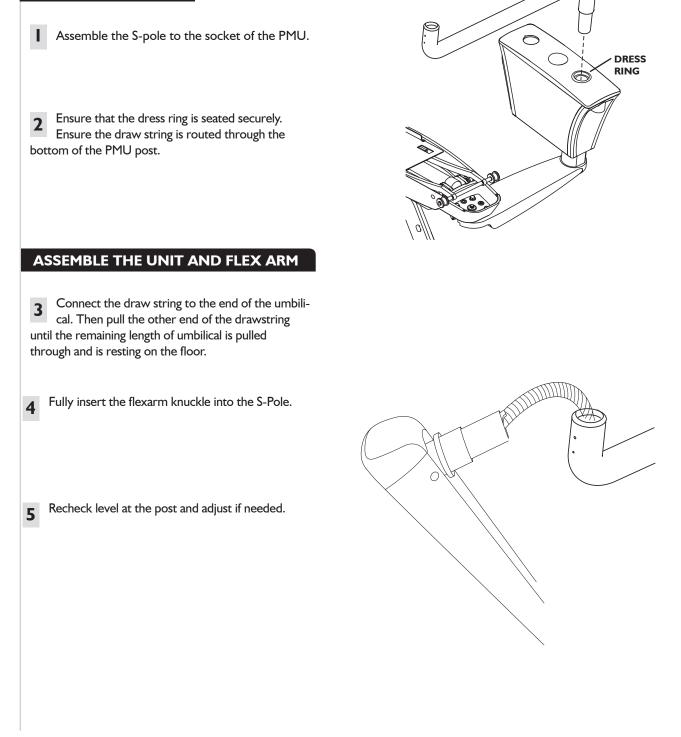

PMU MOUNT UMBILICAL ROUTING

PREPARATION

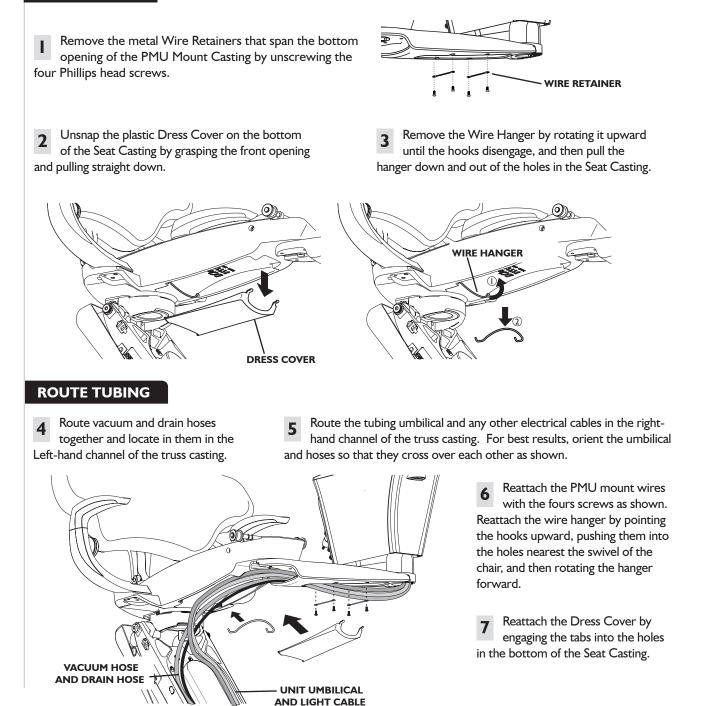

Proceed to the section: MANAGING THE UMBILICAL, page 13


SWING MOUNT UNIT INSTALLATION

TOOLS NEEDED FOR INSTALLATION

Socket wrench Socket wrench extension (3") 9/16" and 3/4" Sockets Level Allen wrench

INCLUDED HARDWARE

- 4 Hex bolts 3/8"-16 x 1 1/4"
- 4 Lock washers 3/8"

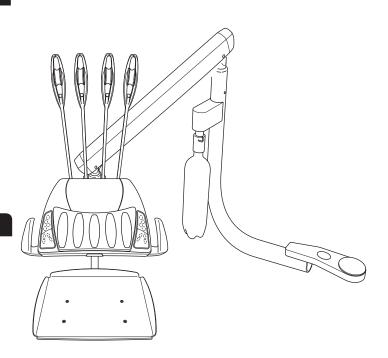

PREPARATION


2

3

Ensure that the dental chair has been completely set up and in its final location.

Remove the shipping bolt from the chair.

Install the power switch cover.

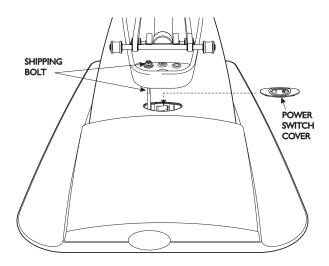

DCI Edge 2

SWING MOUNT UNIT INSTALLATION

MOUNTING TO THE CHAIR

Assemble the hanging bolt and washer to the underside of the seat casting, ensuring that at least 1/2" of the screw thread is exposed as shown.

2 Slide the Swing Mount Casting and Pole Assembly onto the hanging bolt and position it so that it is in line with the seat casting, pointing toward the foot of the chair.

3 Align the holes of the Swing Mount casting to the 4 holes of the seat casting. Assemble the 4 bolts from above by dropping them through the four holes in the seat casting as shown (right) and turn them in part way by hand.

Tighten using a 9/16" socket wrench with a socket extension.


5 Measure the level by attaching a magnetic level to the back of the vertical portion of the inner bent pole and then again at the side of the same pole.


6 Adjust the level by loosening the 4 bolts by 2 full turns or more and then tightening the 3 set screws circled in the illustration (right) as needed. Retighten the 4 bolts and recheck the level.

7 Complete the process by tightening the bottom Hanging Bolt with a 3/4" socket to secure the leveling.



WARNING: To prevent injury, have an assistant support the weight of the unit and mount casting during installation.

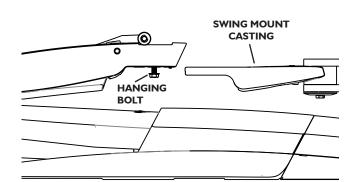

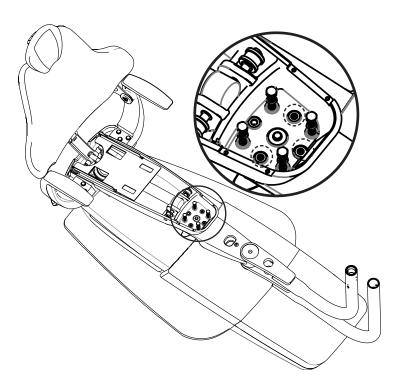




WARNING: Before using of the equipment, ensure that the assembly is level and all mounting bolts are securely fastened.

SWING MOUNT UNIT INSTALLATION

ASSEMBLE THE UNIT AND FLEX ARM


Connect the draw string to the end of the umbilical as shown below. Then pull the other end of the drawstring until the remaining length of umbilical is pulled through and is resting on the floor.

- **2** Fully insert the flexarm knuckle into the S-Pole.
- **3** Recheck level at the post and adjust if needed.

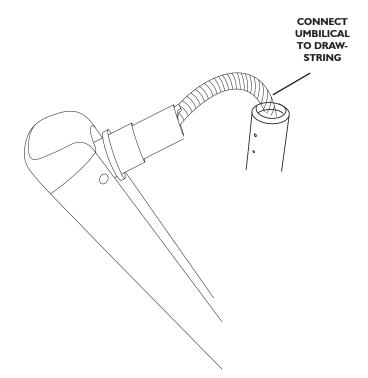

SWING MOUNT UMBILICAL ROUTING

PREPARATION

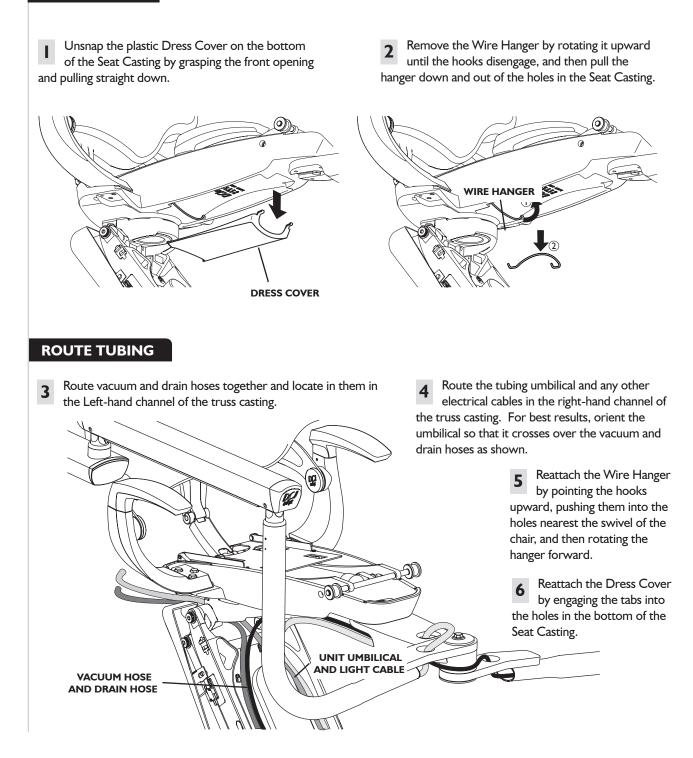


DCI Edge

MANAGING THE UMBILICAL

TRUSS AND PUMP AREA

Manage tubing using the preinstalled managing loops in the truss, making sure to leave tubings loose enough for the chair to raise and lower as well as swivel freely without being stretched or pinched.

2 Against the side of the transformer box, manage the unit umbilical and all wires using the preinstalled loops as shown below.




JUNCTION BOX POSITION


3 Determine the position of the Junction Box in front of the chair (see next page for details). Cut the large corrugated tubing to the appropriate length so that it can extend from the exit hole in the front of the chair to the entrance hole of the Junction Box, allowing 3 inches extra at each end for clamping.

4 Disconnect the power supply harness from the front of the power supply, then using a #2 Phillips screwdriver, remove the strain relief from the side of the power supply. Route the power supply harness through the corrugated tubing (wall connector will not fit through tubing) then re-install the strain relief and reconnect the power supply harness.

5 Pass the remainder of the umbilical through the large corrugated tubing and use the included clamp to secure it as it exits the chair.

6 Insert the corrugated tubing into the lower half of the junction box frame and secure with the included tie wrap as shown.

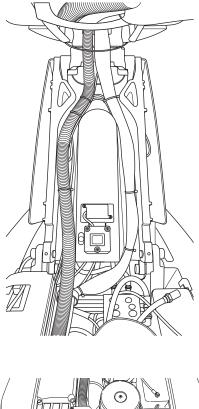

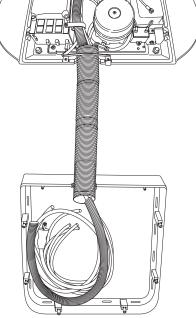

JUNCTION BOX LAYOUT

LOCATE JUNCTION BOX

New: Locate utilities in the operatory according to the dimensions shown for new installations. The junction box should be aligned to the front of the chair where possible.

Existing: For preexisting locations, the junction box can be positioned where necessary. Cut umbilical tubing after determining proper position of the junction box.

Position utilities according to recommended layout as shown where possible.

AIR

Pipe: 1/2" N.P.T. Protruding 1" from the floor. Supplied by contractor.

Air supply: Pressure 80-100psi. Air should be free from contaminants.

WATER

Pipe: 1/2" N.P.T. Protruding 1" from the floor. Supplied by contractor.

Water supply: Pressure 40-80psi. Water should be flushed clean before connecting to this equipment.

ELECTRICAL


Pipe: 1/2" conduit with dual receptacle box or greater. Supplied by contractor. Wire box according to code. Top of box should be no higher than shown. **Supply:** 115V AC 3-wire, 8 AMP or 230V AC 3-wire, 4 AMP

CENTRAL VACUUM


Pipe: Supplied by contractor. Terminated with 5/8" OD tube protruding 1" from the finished floor.


GRAVITY DRAIN

Pipe: 5/8" OD tube protruding I" from the floor. Place trap in-line and use vented fitting to conform to local codes. Supplied by contractor.

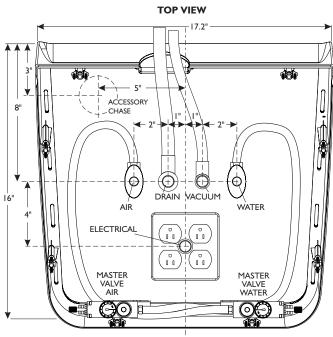


FRONT VIEW

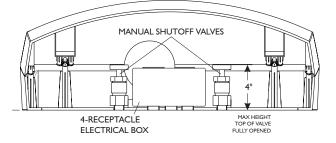

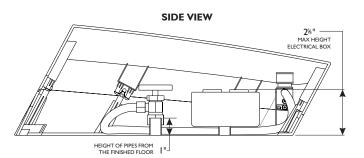

MAKE CONNECTIONS AND ADJUSTMENTS

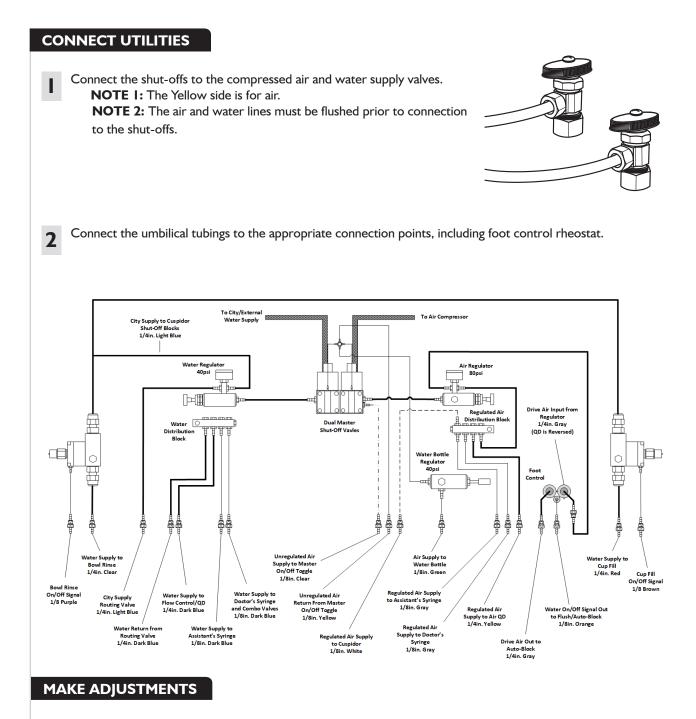

See the ADJUSTMENTS section near the end of the **Instructions for Use** Manual for the **SERIES 5 Euro-Style Delivery System** to complete the installation. Be sure to check and make any needed adjustments to items in that section.

CE PN 50144, Rev. C. 2022-12-06

www.dcionline.com 800-624-2793



705 S. Springbrook Road Bdlg C Newberg, OR 97132, USA